

Calibration of Gauge Block Comparators

PURPOSE

This document has been produced by EAL to improve the harmonisation in gauge block calibration. It provides guidance to national accreditation bodies to set up minimum requirements for the calibration of gauge block comparators and gives advice to calibration laboratories to establish practical procedures.

EAL-G21 * CALIBRATION OF GAUGE BLOCK COMPARATORS

Authorship

This publication has been revised by EAL Committee 2 (Calibration and Testing Activities), based on the draft produced by the EAL Expert Group on Dimensional Metrology.

Official language

The text may be translated into other languages as required. The English language version remains the definitive version.

Copyright

The copyright of this text is held by EAL. The text may not be copied for resale.

Guidance Publications

This document represents a consensus of EAL member opinion and preferred practice on how the relevant clauses of the accreditation standards might be applied in the context of the subject matter of this document. The approaches taken are not mandatory and are for the guidance of accreditation bodies and their client laboratories. Nevertheless, the document has been produced as a means of promoting a consistent approach to laboratory accreditation amongst EAL member bodies, particularly those participating in the EAL Multilateral Agreement.

Further information

For further information about this publication, contact your National member of EAL:

	Calibration National member	Testing National member
Austria	BMwA	BMwA
Belgium	BKO/OBE	BELTEST
Denmark	DANAK	DANAK
Finland	FINAS	FINAS
France	COFRAC	COFRAC
Germany	DKD	DAR
Greece	Ministry of Commerce	ELOT
Iceland	ISAC	ISAC
Ireland	NAB	NAB
Italy	SIT	SINAL
Netherlands	RvA	RvA
Norway	NA	NA
Portugal	IPQ	IPQ
Spain	ENAC	ENAC
Sweden	SWEDAC	SWEDAC
Switzerland	SAS	SAS
United Kingdom	UKAS	UKAS

Contents

Section	Page
1 Introduction	4
2 Scope and field of application	4
3 Terminology	4
4 Reference standards	5
5 Example of a calibration procedure	6
6 Evaluation of results	7
7 Measurement uncertainty	8
8 Calibration certificate	8
9 References	9
Appendix A	10

1 Introduction

- 1.1 The purpose of this technical guideline is to improve the harmonisation within EAL for gauge block calibration. It provides guidance to national accreditation bodies to set up minimum requirements for the calibration of gauge block comparators and gives advice to calibration laboratories to establish practical procedures. The guideline is based on a national calibration guideline [ref. 1] and on the International Standard ISO 3650 [ref. 2]. In the first part (sections 2, 3 and 4), the general definitions and the minimum technical requirements for the calibration of gauge block comparators are given. The second part of this guideline is of procedural nature and gives practical advice to calibration laboratories. In sections 5 and 6 an example of a typical calibration procedure is presented. It may be amended or modified to meet the specific requirements of accreditation.

2 Scope and field of application

- 2.1 This guideline refers to instruments used to calibrate gauge blocks up to 100 mm nominal length by the comparison method (cf. ISO 3650, clause 7.4), where the length of a standard gauge block is transferred to the gauge block under test by mechanical probing. The calibration shall be carried out with the aid of gauge blocks. The guideline is intended only for instruments probing the measurement faces of the gauge block with two length indicators from opposite sides.
- 2.2 **Components:** The gauge block comparator comprises the measurement pedestal, the measurement table with the gauge block positioning device, two length indicators connected to an electronic measuring instrument with numerical display and a digital interface, if necessary.
- 2.3 **Site of calibration:** The comparator shall be calibrated at the place of use, so that all the ambient conditions which will influence the instrument in service, are taken into consideration.

Note: General requirements for the accreditation of laboratories and organisations performing site calibrations are given in Publication EAL-R3. [ref. 3]

3 Terminology

- 3.1 The definitions used in this guideline are in compliance with the International Standard ISO 3650 [ref. 2].

l_n nominal length of the gauge block

l_c central length of the gauge block

$f_o = l_{\max} - l_c$ difference between maximum length and central length


$f_u = l_c - l_{\min}$ difference between central length and minimum length

The variation of length measured at the centre and the four corners of the gauge block can be regarded as representative for f_o and f_u (ISO 3650, clause 7.4.4).

4 Reference standards

4.1 The gauge block comparator shall be calibrated by means of gauge blocks, preferably using 6 pairs of typically the following lengths:

Pair No.	Nominal length / mm	
	A	B
1	0,5	0,5
2	1,0	1,005
3	1,0	1,01
4	4,0	4,0
5	100,0	100,0
6	6,0	6,0*

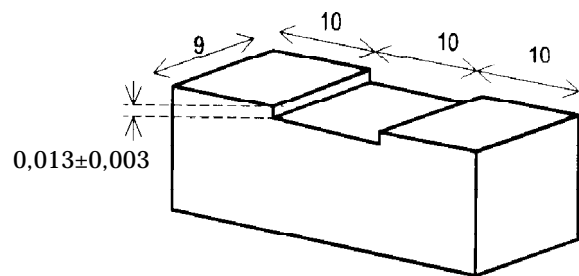

* bridge-shaped gauge block

4.2 The gauge blocks shall all be of the same material, marked with an identification number and satisfy with respect to the quality of the measurement faces (flatness and variation in length) the tolerances of the calibration grade K (ISO 3650). Gauge block B of pair No. 6 is a special block designed as a bridge. It allows the sensitivity of the lower length indicator to be compared with the sensitivity of the upper indicator. One of its measuring faces is flat whereas the opposite face is divided into three sections of almost equal size (9 mm x 10 mm). The centre section has a nominal length of 6 mm, the two outer sections are $(13 \pm 3) \mu\text{m}$ longer. The plane measuring face of the gauge block must have wringing quality. The variation in length should not exceed $0,05 \mu\text{m}$ in the central area (7 mm in diameter) and $0,2 \mu\text{m}$ on the protruding sections. Such bridge-shaped gauge blocks are commercially available from several manufacturers.

4.3 The difference between the central lengths l_c of gauge blocks A and B forming pairs 1 to 5, and the deviations f_o and f_u from the central length of gauge blocks B of pairs 2 and 3 shall be calibrated with an expanded uncertainty of measurement ($k = 3$) preferably smaller than or equal to $0,015 \mu\text{m}$. The gauge blocks of pair No. 6 need not be calibrated.

5 Example of a calibration procedure

5.1 Preparation for calibration

- 5.1 Before calibration, check that the gauge block comparator operates correctly as described in the manufacturer's operating instructions. In addition, the following properties shall be checked:
- (a) The surface of the measurement table must be impeccable, i.e. without scratches and wear.
 - (b) The measuring faces of the anvils must be undamaged and spherical. Their vertices must be correctly aligned with respect to each other.
 - (c) The measuring force of the upper and lower length indicators must be in compliance with the manufacturer's specifications.
 - (d) The correct sequence for the retraction of the two anvils. The measuring face of the lower anvil must be retracted below the surface of the measurement table.
 - (e) In the non-lowered position, the measuring face of the lower anvil shall protrude from the measurement table's surface by 20 μm to 100 μm .

5.2 Comparison measurement of central length


- 5.2.1 With each of the gauge block pairs Nos. 1 to 5, five comparison measurements shall be carried out. The measurements shall be repeated after the positions of gauge blocks A and B have been interchanged in the gauge block positioning device. The mean values and the standard deviations shall be calculated for each measurement series of a pair of gauge blocks (10 measurement values).

5.3 Comparison measurement with the bridge shaped gauge block

- 5.3.1 Two measurement series, each comprising 10 measurements, shall be carried out for pair No. 6. In the first series, the bridge shaped gauge block shall be placed with the plane measuring face on the measuring table, whereas for the second series it is turned upside down. The mean values and the standard deviations shall be calculated for both measurement series (10 measurement values each) as well as the difference between the two mean values.

5.4 Deviations f_o and f_u from the central length

- 5.4.1 To determine the deviations f_o and f_u from the central length, each of the four corners of the measuring face of one of the gauge blocks 1,005 mm or 1,01 mm shall be probed five times in succession, starting at the centre of the measuring face.

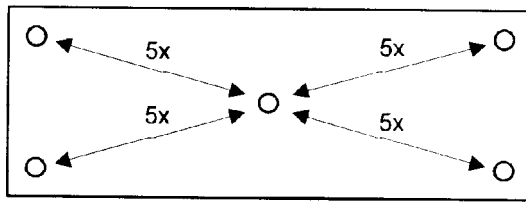

The four measurement series shall be repeated after the gauge block being rotated by 180° in the horizontal plane. The mean values and the standard deviations shall be calculated for each of the eight measurement series. The deviations f_o

and f_u from the central length result from the largest and the smallest value of the eight mean values.

6 Evaluation of results

6.1 General consideration

6.1.1 In principle, the measurement results and the calibration values of the standards can be used to determine corrections for the calibrated comparator and to estimate the uncertainty. In practice, however, the indicated values of the comparator are used without correction to simplify the measurement procedure. This is justifiable, as the measured length differences are small and the corrections can be ignored in general. Their influence shall be taken into account as a contribution to the uncertainty. In cases, where the deviations of the indicated values exceed acceptable limits, the comparator and its electronics should be readjusted.

6.1.2 In the following, criteria for acceptance of the gauge block comparator are given and the uncertainty based on these criteria is stated. These criteria are recommended to be applied for high accuracy calibrations of grade 0 gauge blocks, where a target expanded measurement uncertainty of typically

$$0,05 \mu\text{m} + 0,5 \times 10^{-6} \times l_n (k = 2)$$

is aimed at. If these criteria are not met or if higher uncertainties are tolerable, the criteria may be modified and the associated uncertainty has to be evaluated.

6.2 Acceptance criteria

6.2.1 The standard deviations determined according to paragraphs 5.2, 5.3 and 5.4 shall not exceed the value of 0,015 μm . The maximum permissible deviation of the mean values according to paragraph 5.2, and the maximum permissible deviation of the values f_o and f_u according to paragraph 5.4 from the values according to the calibration certificate of the standards amount to $\pm 0,03 \mu\text{m}$. The difference between the mean values according to paragraph 5.3 shall not exceed $\pm 0,03 \mu\text{m}$.

7 Measurement uncertainty

- 7.1 Based on the above acceptance criteria, the measurement uncertainty of the gauge block comparator has been evaluated. Taking into account the random contribution for an average of at least five single measurements, the digital resolution of the electronic indicator (0,01 μm), a residual difference in the sensitivity of the two length indicators, the quality of the measuring table and the uncertainty of calibration of the length indicators, one obtains an expanded uncertainty of $U = 0,03 \mu\text{m} + 0,002 \times D$, if the indicated length difference D does not exceed 10 μm . The stated uncertainty corresponds to the combined standard uncertainty multiplied by the coverage factor $k = 2$, in accordance with EAL-R2 [ref. 4].
- 7.2 The uncertainty of the gauge block comparator has to be taken into account, when the uncertainty of gauge block calibration is evaluated. It does not contain the influence of temperature and the quality of the measuring faces of the gauge blocks to be compared.

8 Calibration certificate

- 8.1 The certificate of calibration shall be in conformance with EAL-R1 [ref.5]. In particular it has to contain the following information:
- (a) The place of calibration and of use of the instrument.
 - (b) The identification of the standards used together with their values according to the calibration certificate.
 - (c) The manufacturer, type and serial number of the components of the gauge block comparator.
 - (d) The settings of the control elements of the electronic length measuring instrument during calibration (measuring range, digital resolution of the display etc.).
 - (e) The ambient temperature range during the calibration.
 - (f) The measurement results should be presented in tabular form (see Appendix).

9 References

1. DKD - R4 - 1: 1994. *Auswahl und Kalibrierung von Endmaßmeßgeräten zur Verwendung als Normalgeräte in Kalibrierlaboratorien.*
2. ISO 3650:1995. *Dimensional measuring instruments - Gauge blocks.*
3. EAL-R3: 1996. *Requirements for the Accreditation of Laboratories and Organisations Performing Site Calibrations.*
4. EAL-R2: 1997 *Expression of the Uncertainty of Measurement in Calibration.*
5. EAL-R1: 1995. *Requirements Concerning Certificates Issued by Accredited Calibration Laboratories.*

Appendix A

Example of tables to present the calibration results of a gauge block comparator

A1 Differences of central length l_c

Pair No	Nominal length		Ident. No. of gauge blocks	Value from calibration certificate C $(B - A) / \mu\text{m}$	Measured mean value M $(B - A) / \mu\text{m}$	Difference $C - M$ μm	Measured standard deviation $(B - A) / \mu\text{m}$
	A mm	B mm					
1	0,5	0,5					
2	1,0	1,005					
3		1,010					
4	4	4					
5	100	100					

A2 Difference of central length of pair No. 6

Pair No	Nominal length		Ident. No. of gauge blocks	Measured mean value		Difference of mean μm	Measured standard deviation	
	A mm	B mm		Gauge block B flat side down (Pos. d) $(B - A) / \mu\text{m}$	Gauge block B flat side up (Pos. u) $(B - A) / \mu\text{m}$		Pos. d $(B - A) / \mu\text{m}$	Pos. u $(B - A) / \mu\text{m}$
6	6	6						

A3 Deviations f_o and f_u from the central length

Nominal length mm	Ident. No.	Value from calibration certificate C $f_o \mu\text{m} f_u$		Measured mean value M $f_o \mu\text{m} f_u$		Difference $C - M$ $f_o \mu\text{m} f_u$		Measured standard deviation max. value from 8 series μm